


How to interpret the pH graph

The graph below shows how sensitive the Pi free chlorine sensor is to pH.

The Free Chlorine sensor shows some susceptibility to pH variations above pH 7.

As the pH increases then susceptibility increases.

Very few people need to buffer their chlorine probe. Whether they do or not will depend on what errors are acceptable to them. In practice Pi has sold over 9000 free chlorine sensors and none of them are buffered.

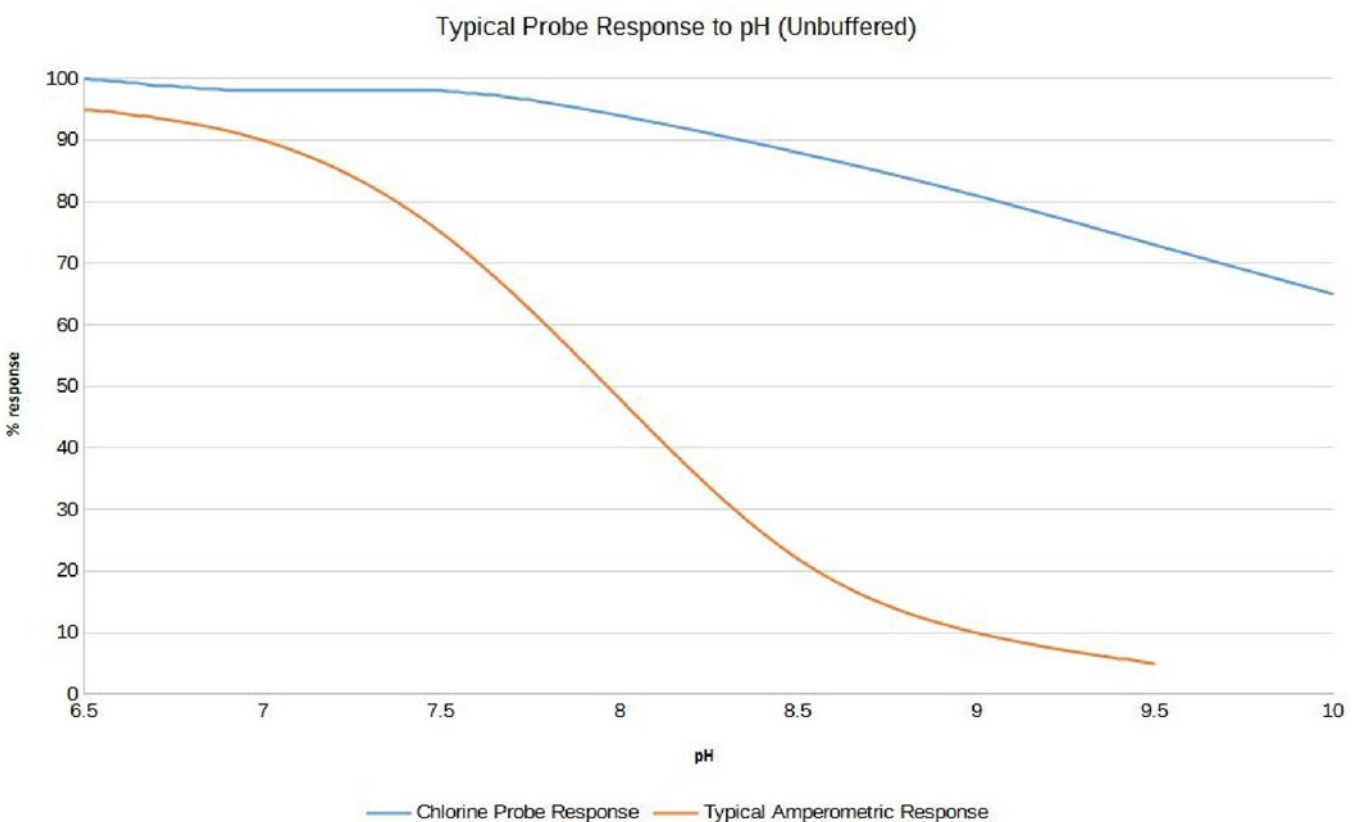

eg. at pH 7

pH varies by +/- 0.1pH

0.5ppm would vary by +/- 0.02ppm
1ppm +/- would vary by +/- 0.02ppm
3ppm +/- would vary by +/- 0.06ppm

pH varies by +/- 0.5pH

0.5ppm would vary by +/- 0.02ppm
1ppm +/- would vary by +/- 0.04ppm
3ppm +/- would vary by +/- 0.12ppm

pH varies by +/- 1pH

0.5ppm would vary by +/- 0.05ppm
1ppm +/- would vary by +/- 0.1ppm
3ppm +/- would vary by +/- 0.3ppm

eg. at pH 8

pH varies by +/- 0.1pH

0.5ppm would vary by +/- 0.02ppm
1ppm +/- would vary by +/- 0.04ppm
3ppm +/- would vary by +/- 0.12ppm

pH varies by +/- 0.5pH

0.5ppm would vary by +/- 0.05ppm
1ppm +/- would vary by +/- 0.1ppm
3ppm +/- would vary by +/- 0.3ppm

pH varies by +/- 1pH

0.5ppm would vary by +/- 0.08ppm
1ppm +/- would vary by +/- 0.15ppm
3ppm +/- would vary by +/- 0.45ppm

eg. at pH 9

pH varies by +/- 0.1pH

0.5ppm would vary by +/- 0.03ppm
1ppm +/- would vary by +/- 0.06ppm
3ppm +/- would vary by +/- 0.18ppm

pH varies by +/- 0.5pH

0.5ppm would vary by +/- 0.07ppm
1ppm +/- would vary by +/- 0.14ppm
3ppm +/- would vary by +/- 0.42ppm

pH varies by +/- 1pH

0.5ppm would vary by +/- 0.16 ppm
1ppm +/- would vary by +/- 0.30 ppm
3ppm +/- would vary by +/- 0.90 ppm

Notes

- These figures are approximate and may vary from probe to probe.
- The effect on the sensor is predictable so that when the pH goes up the probe signal goes down and vice versa.
- When the pH is restored the probe will return to the original value.
- The normally accepted accuracy of a DPD test is +/- 0.06ppm.
- If the free chlorine sensor pH susceptibility is unacceptable, it is possible to correct this by using a pH sensor connected to the analyser and compensate for the pH variation.

Please ask your sales representative for details.

DONT FORGET! 100% of our customers don't use buffers and are very happy with the performance of their chlorine probes.

